

Applicant(s): Jose de la Torre-Bueno

AUTOMATED MEASUREMENT OF CONCENTRATION
AND/OR AMOUNT IN A BIOLOGICAL SAMPLE

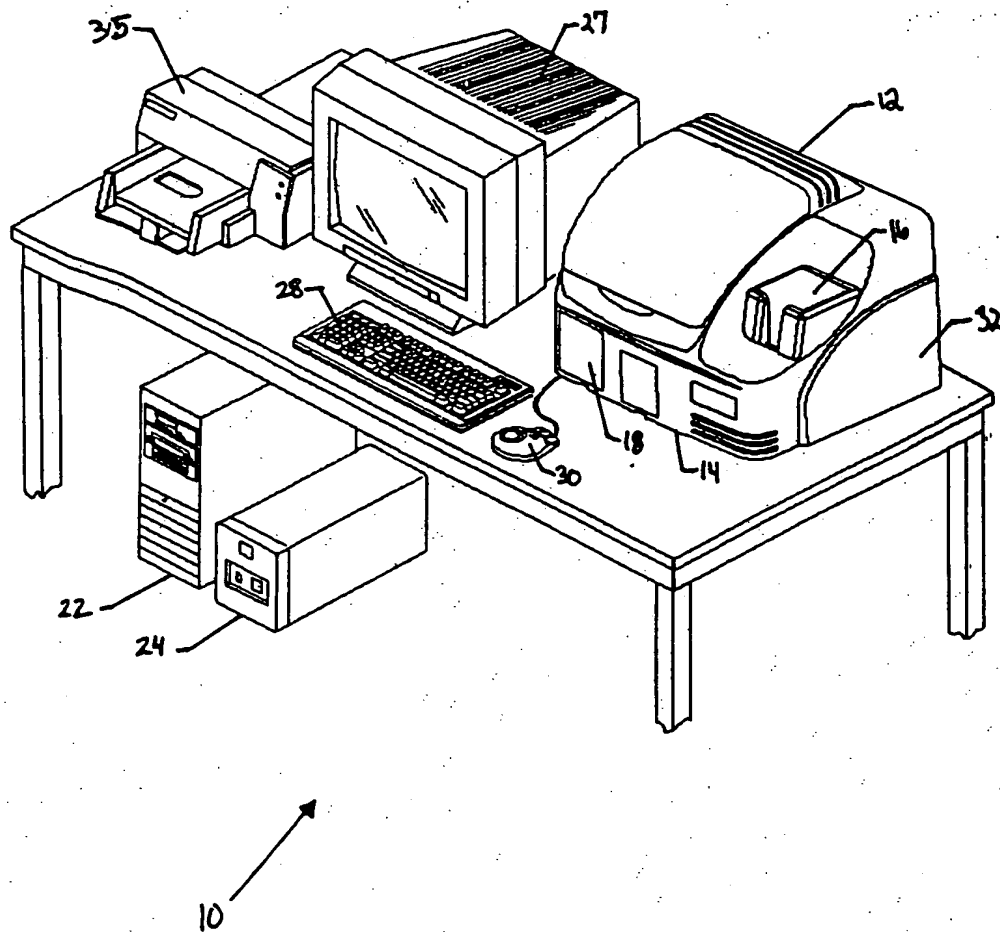


FIG. 1

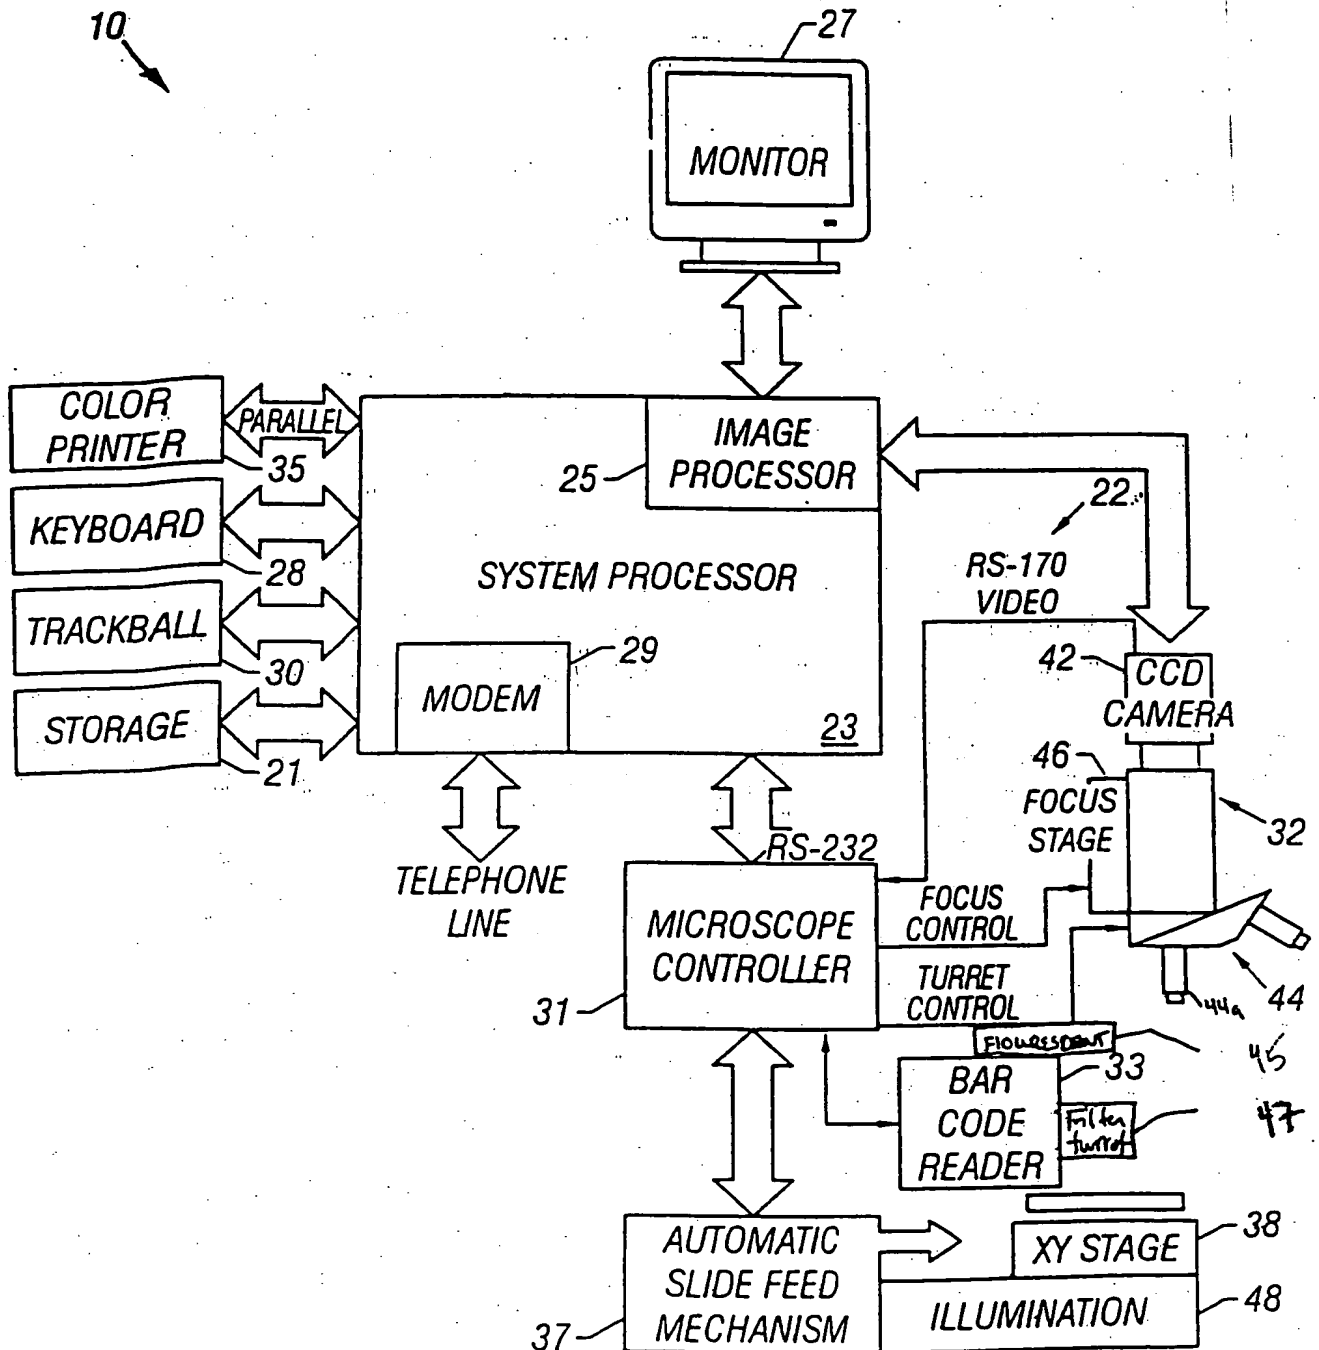


FIG. 2

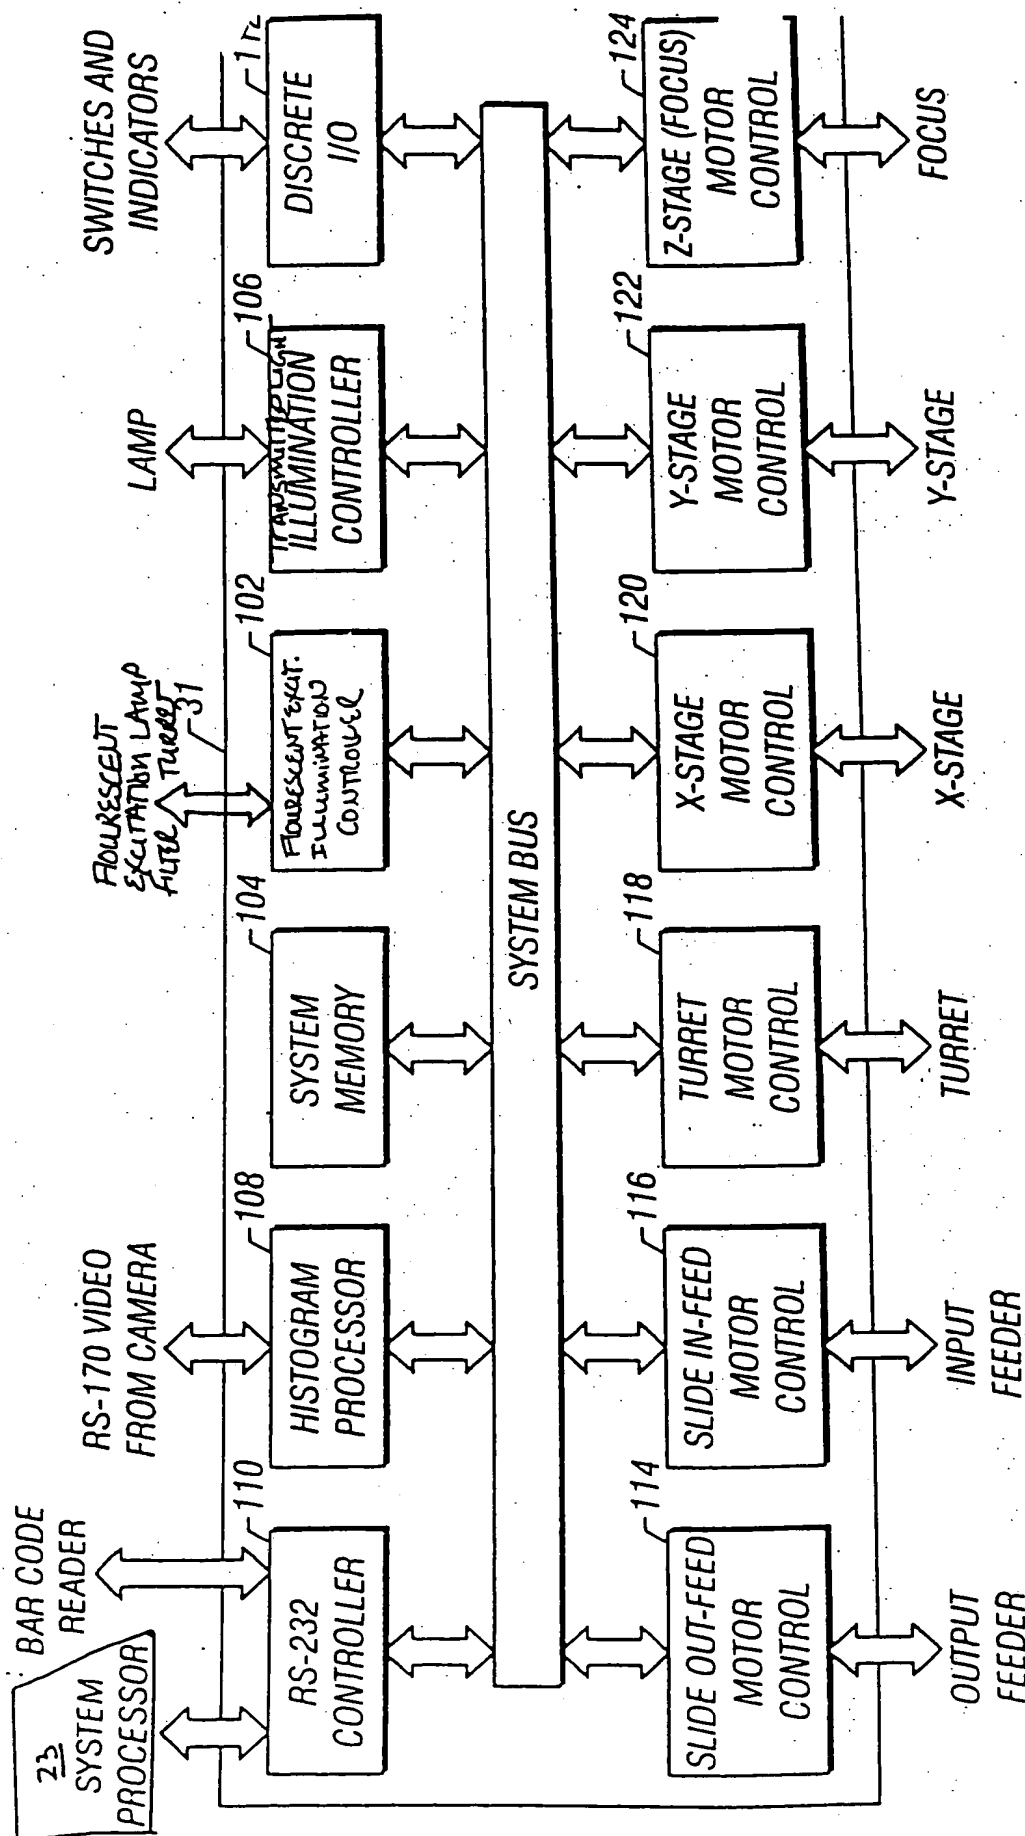


FIG. 3

Applicant(s): Jose de la Torre-Bueno
AUTOMATED MEASUREMENT OF CONCENTRATION
AND/OR AMOUNT IN A BIOLOGICAL SAMPLE

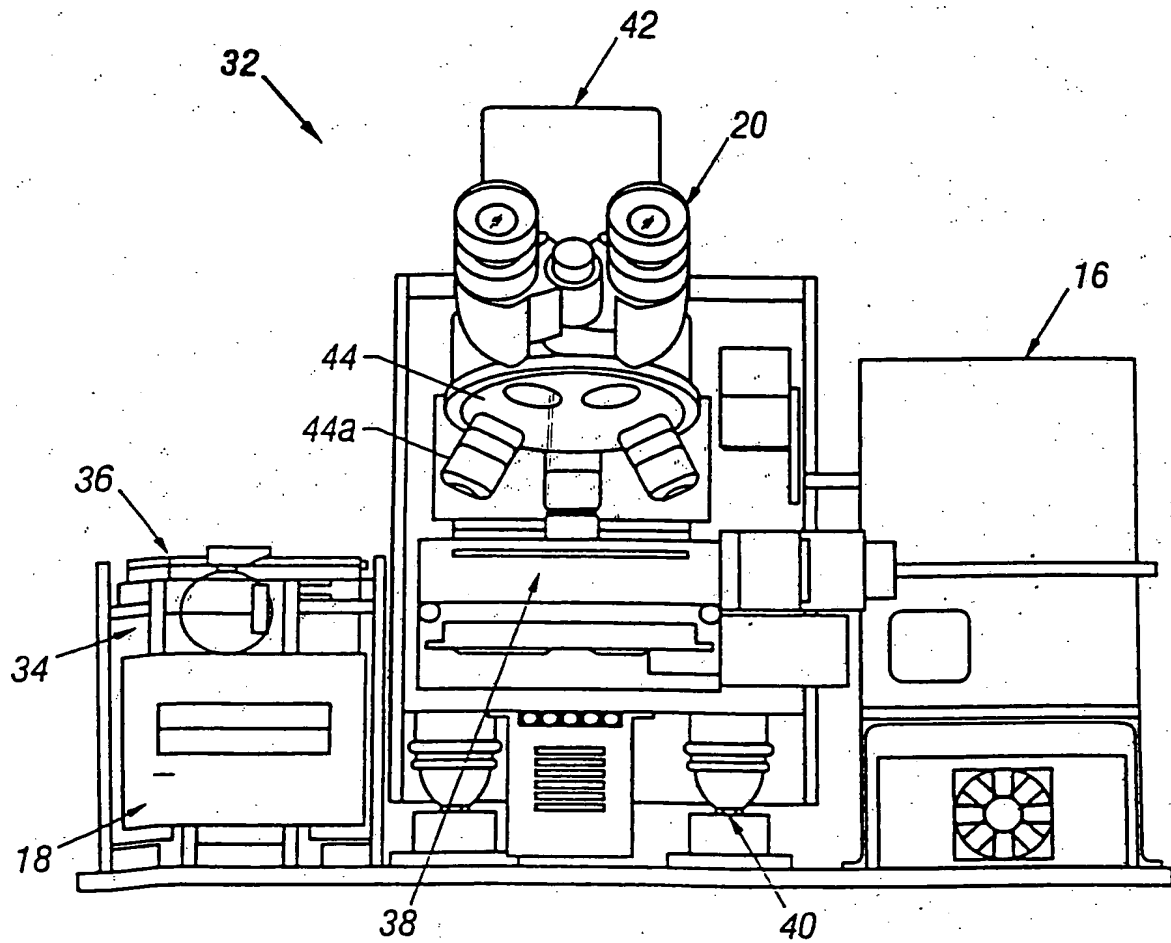


FIG. 4

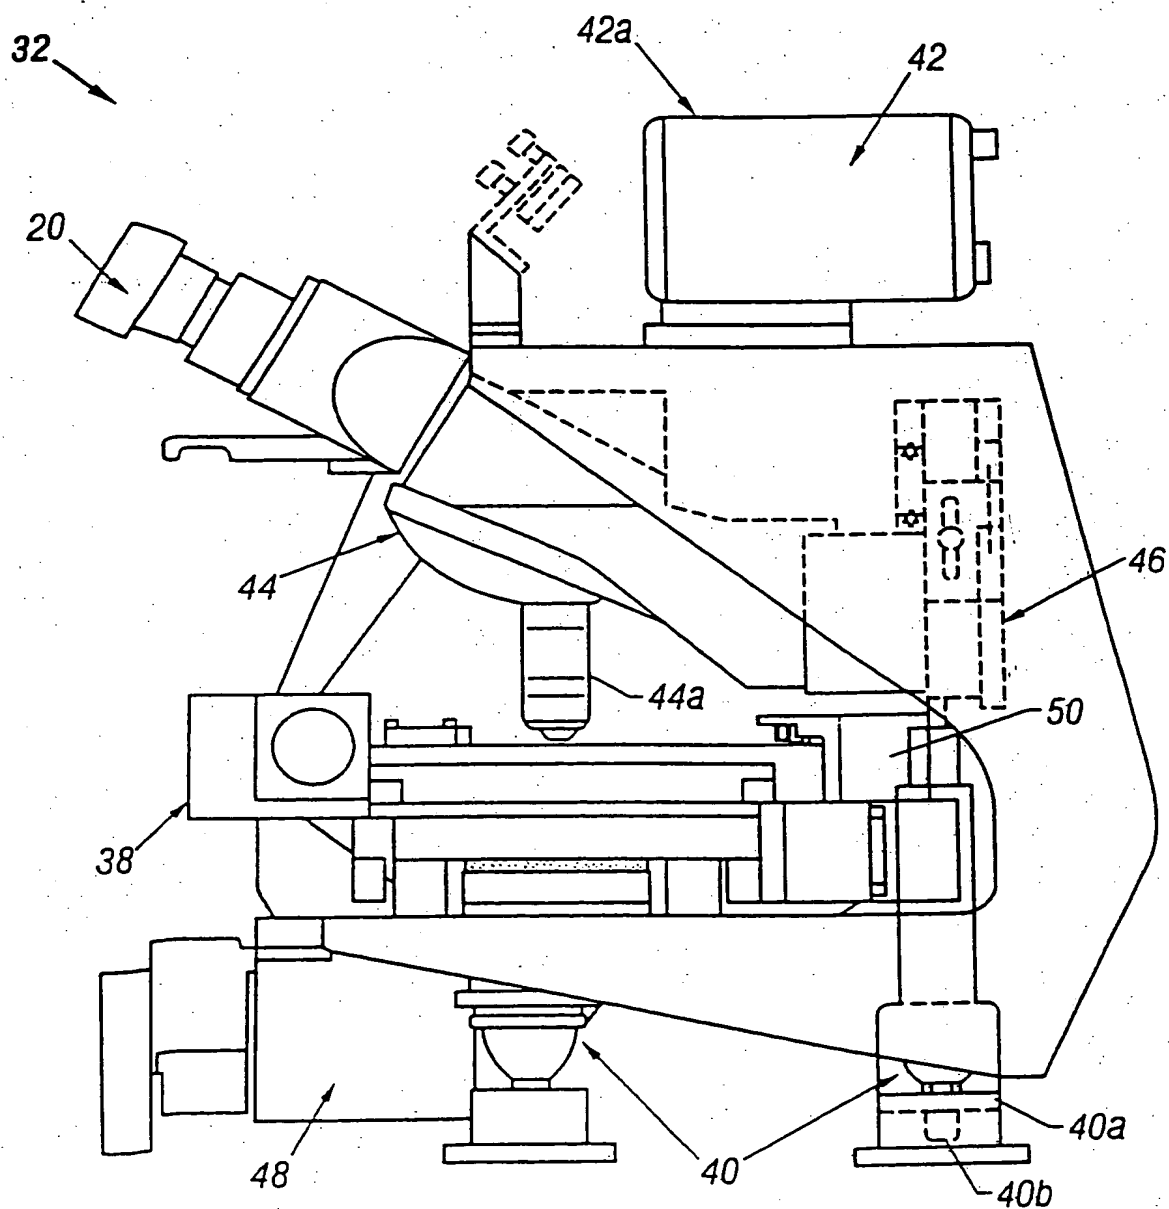


FIG. 5

Applicant(s): Jose de la Torre-Bueno
AUTOMATED MEASUREMENT OF CONCENTRATION
AND/OR AMOUNT IN A BIOLOGICAL SAMPLE



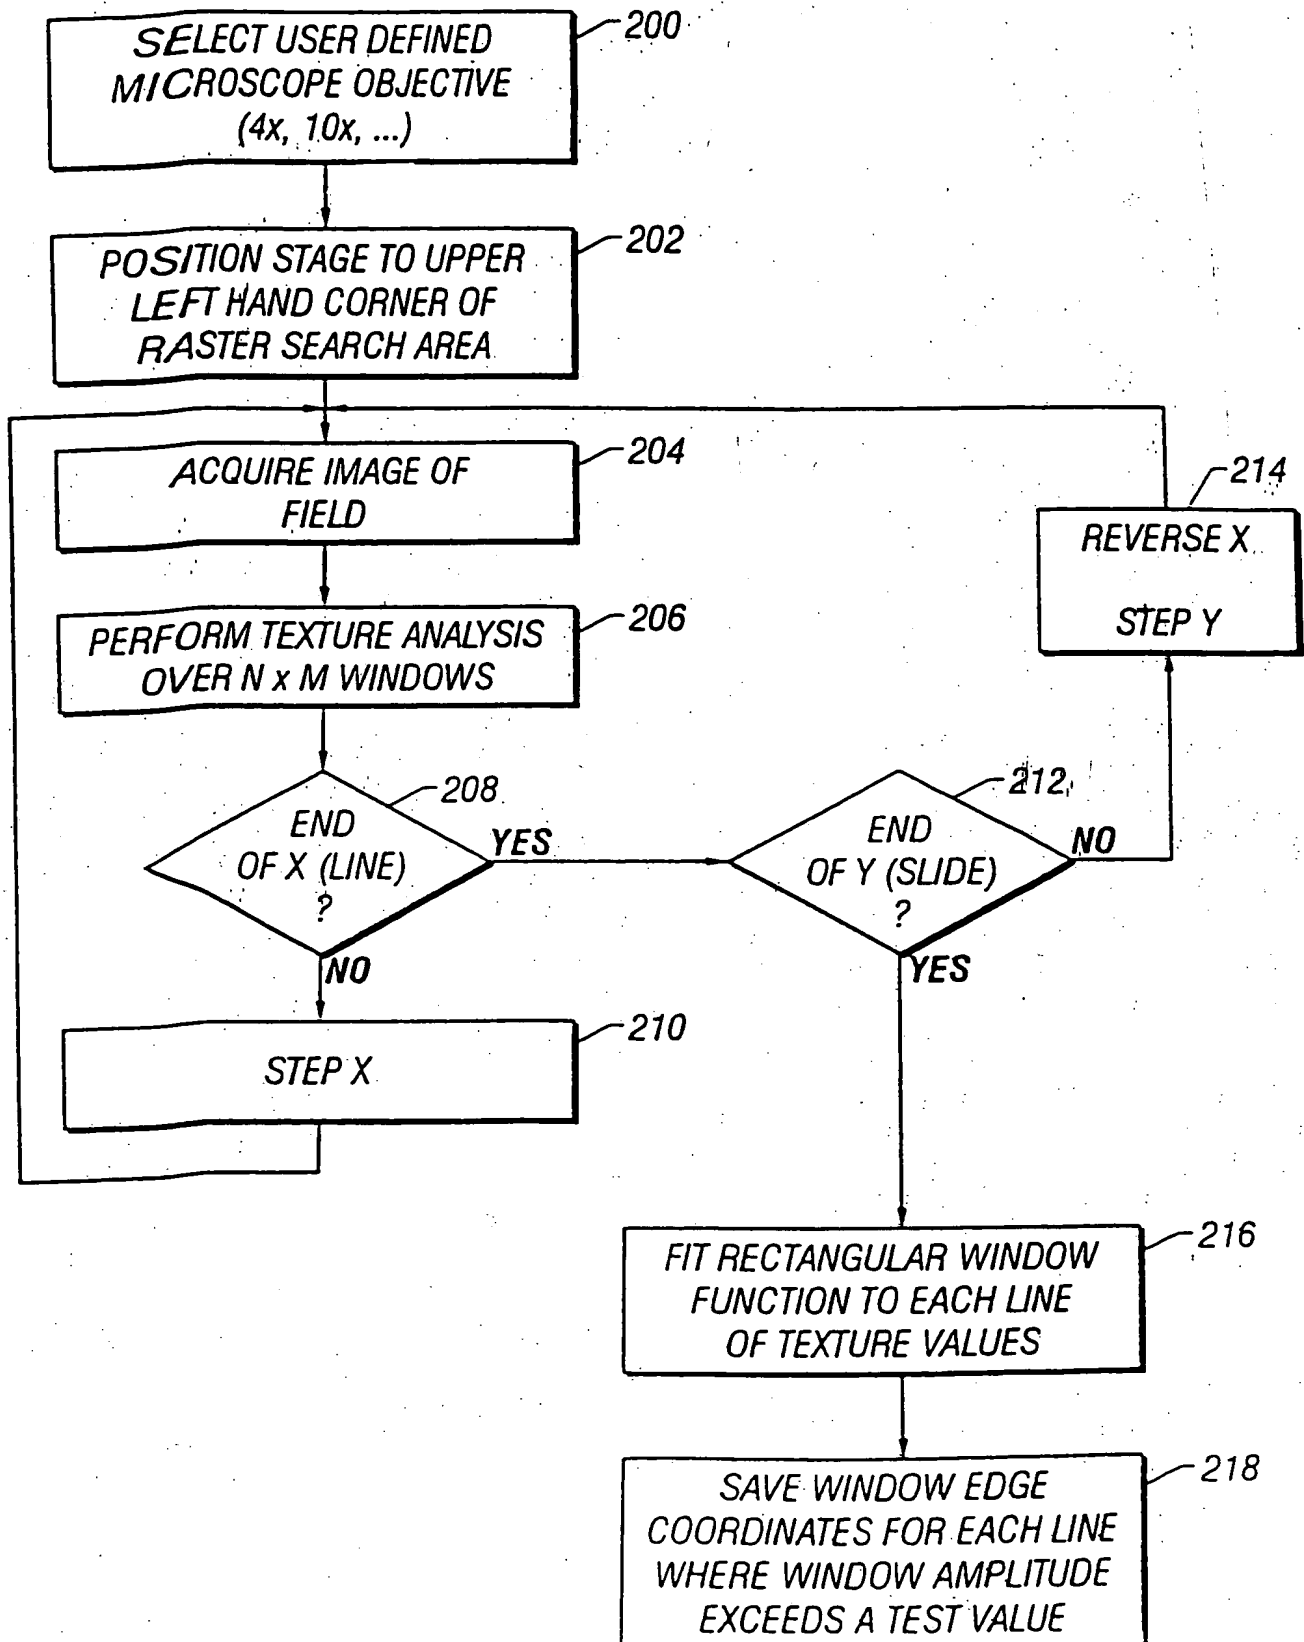


FIG. 6

Applicant(s): Jose de la Torre-Bueno
AUTOMATED MEASUREMENT OF CONCENTRATION
AND/OR AMOUNT IN A BIOLOGICAL SAMPLE

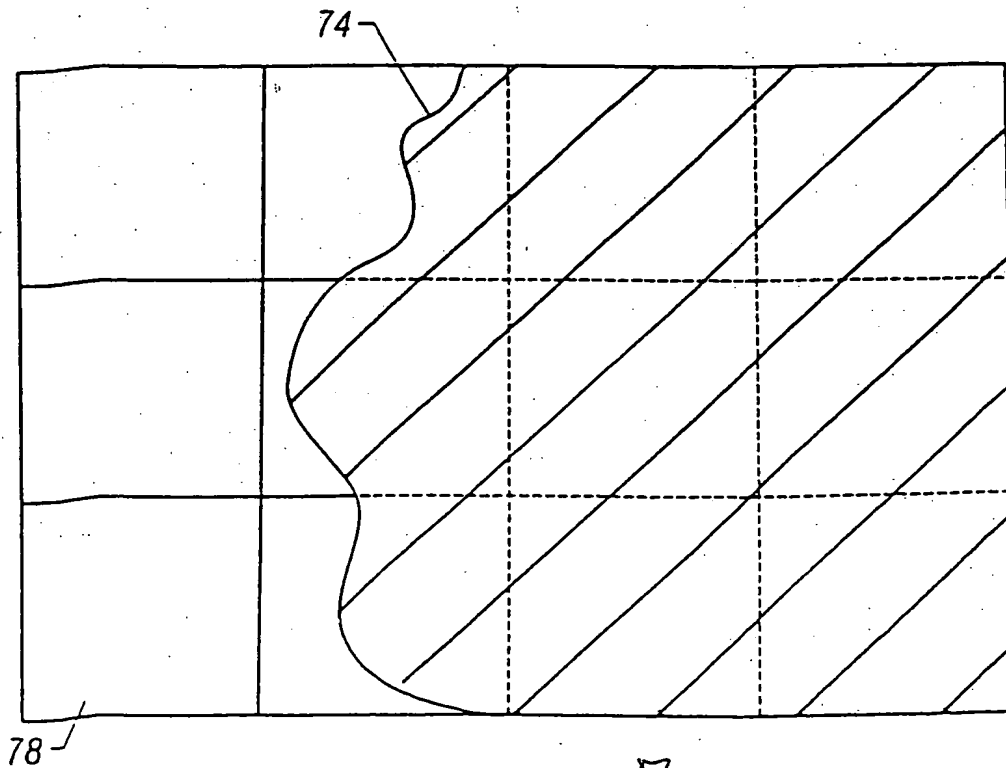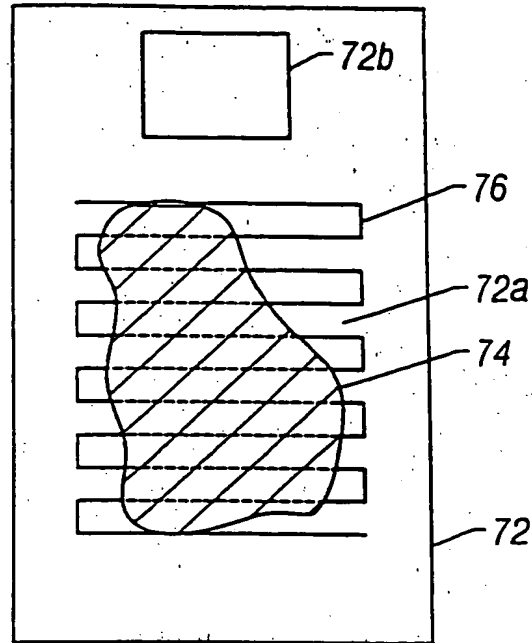

Applicant(s): Jose de la Torre-Bueno
AUTOMATED MEASUREMENT OF CONCENTRATION
AND/OR AMOUNT IN A BIOLOGICAL SAMPLE

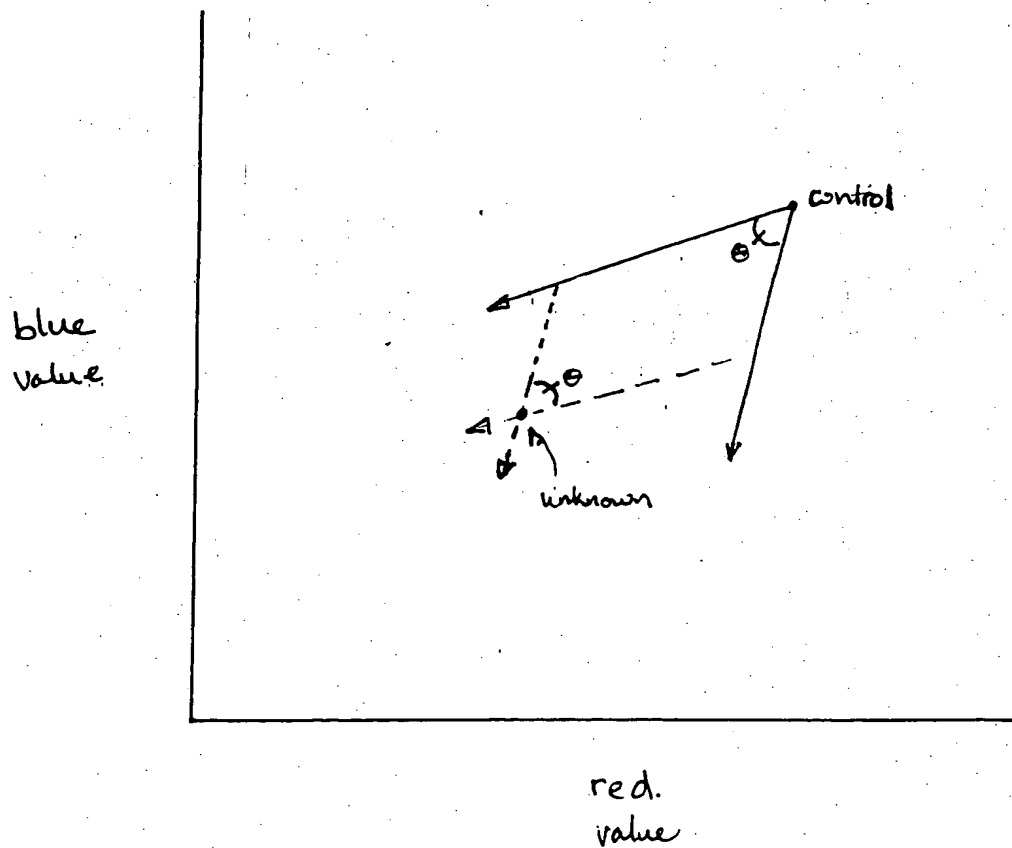


FIG. 9

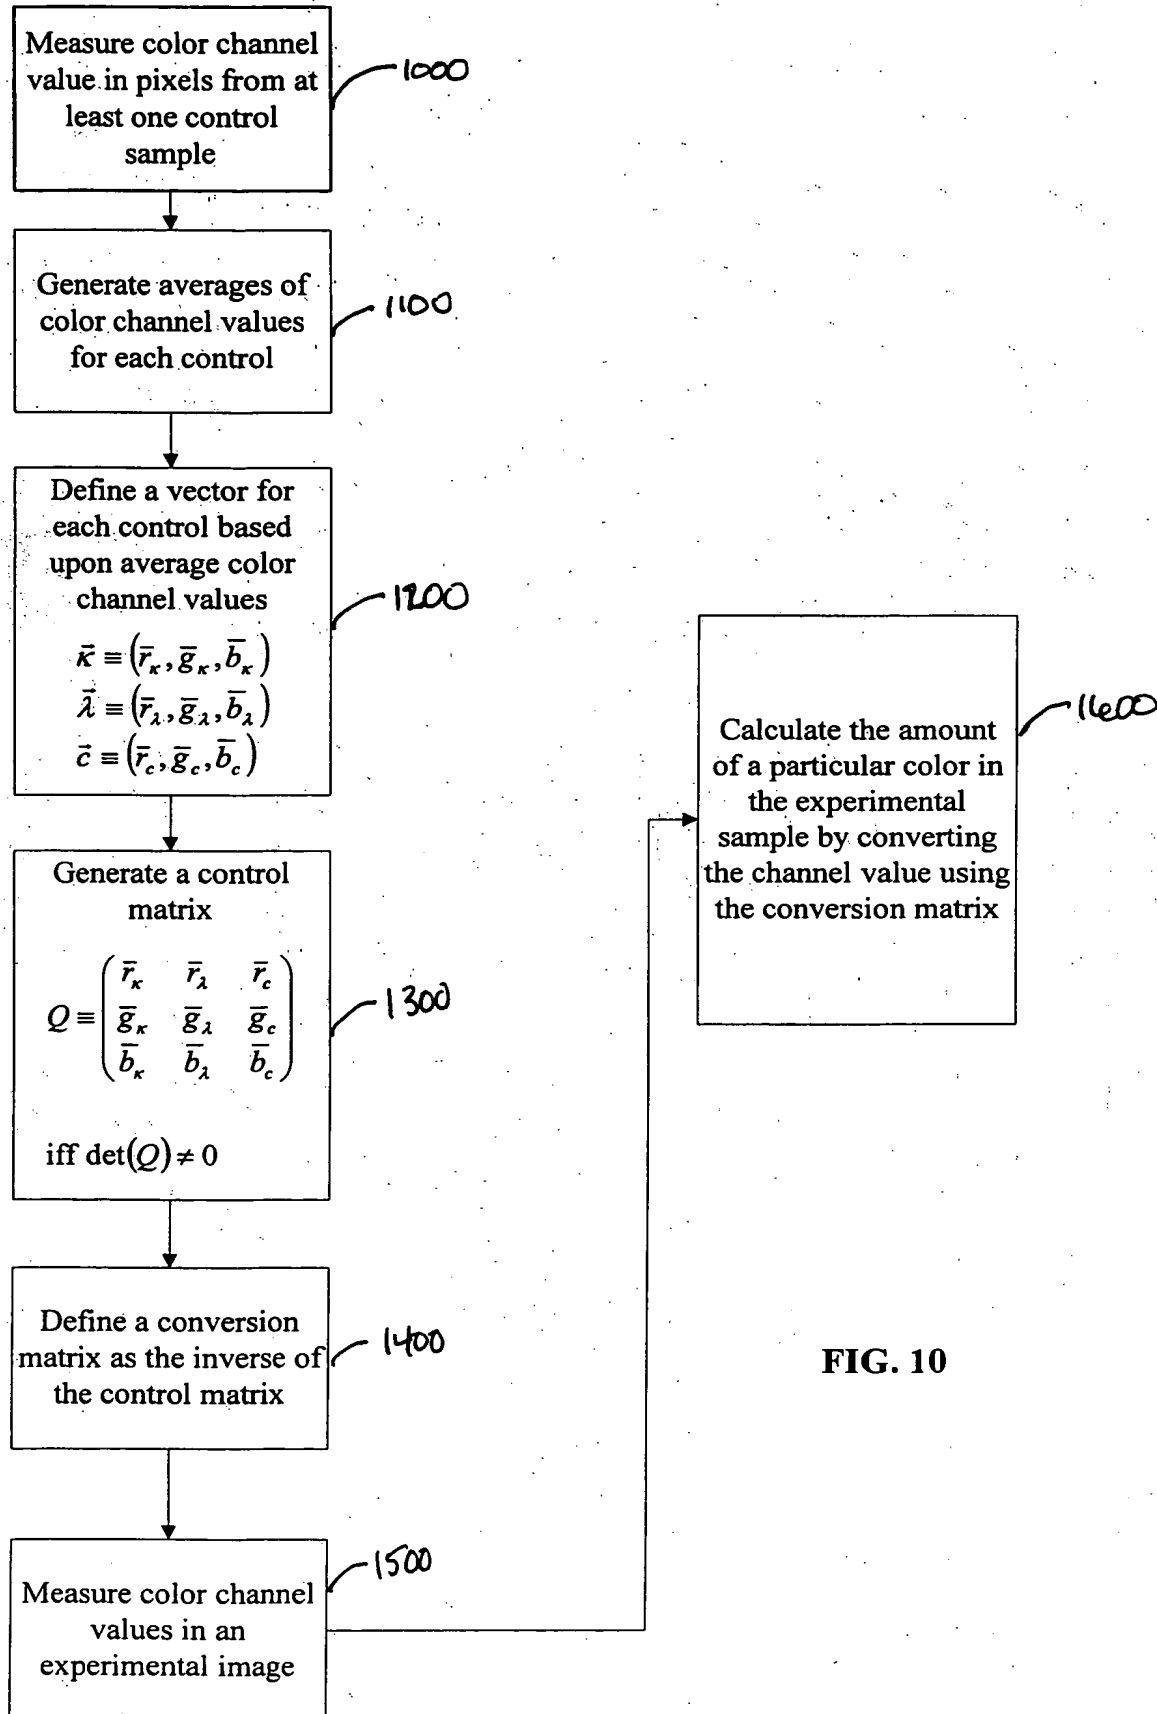


FIG. 10